



TCS Results – water flow open


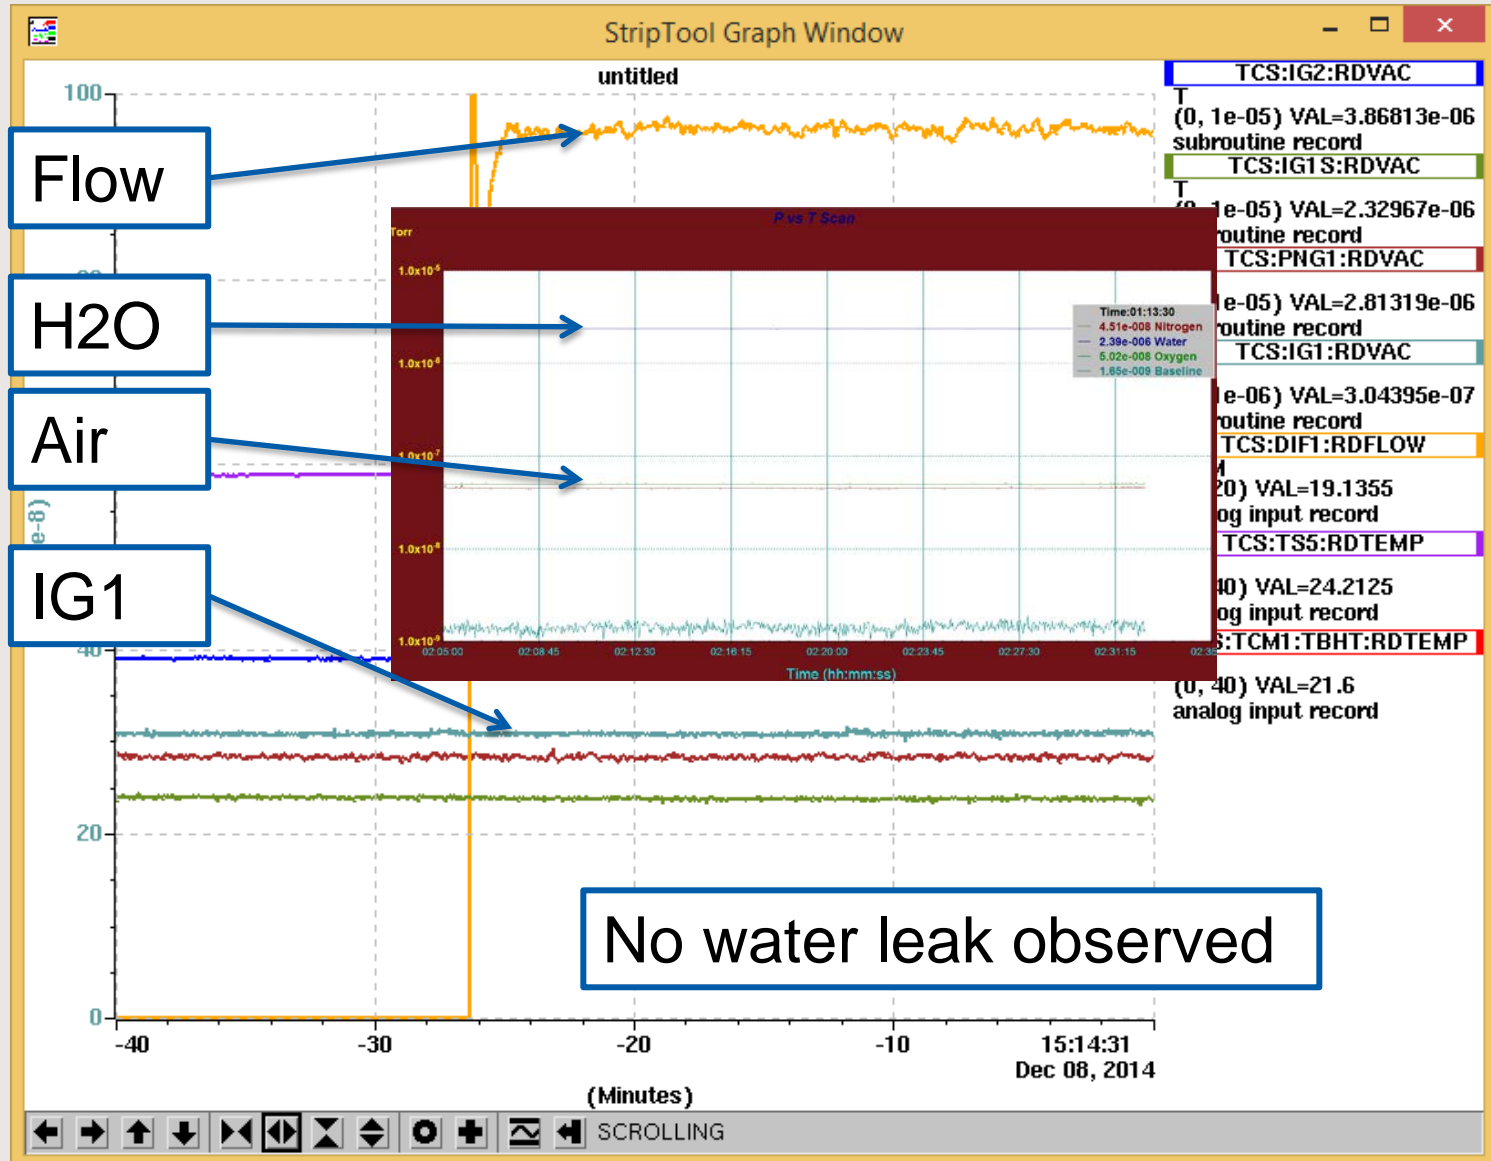


New TCS TGHT and TBHT power supplies

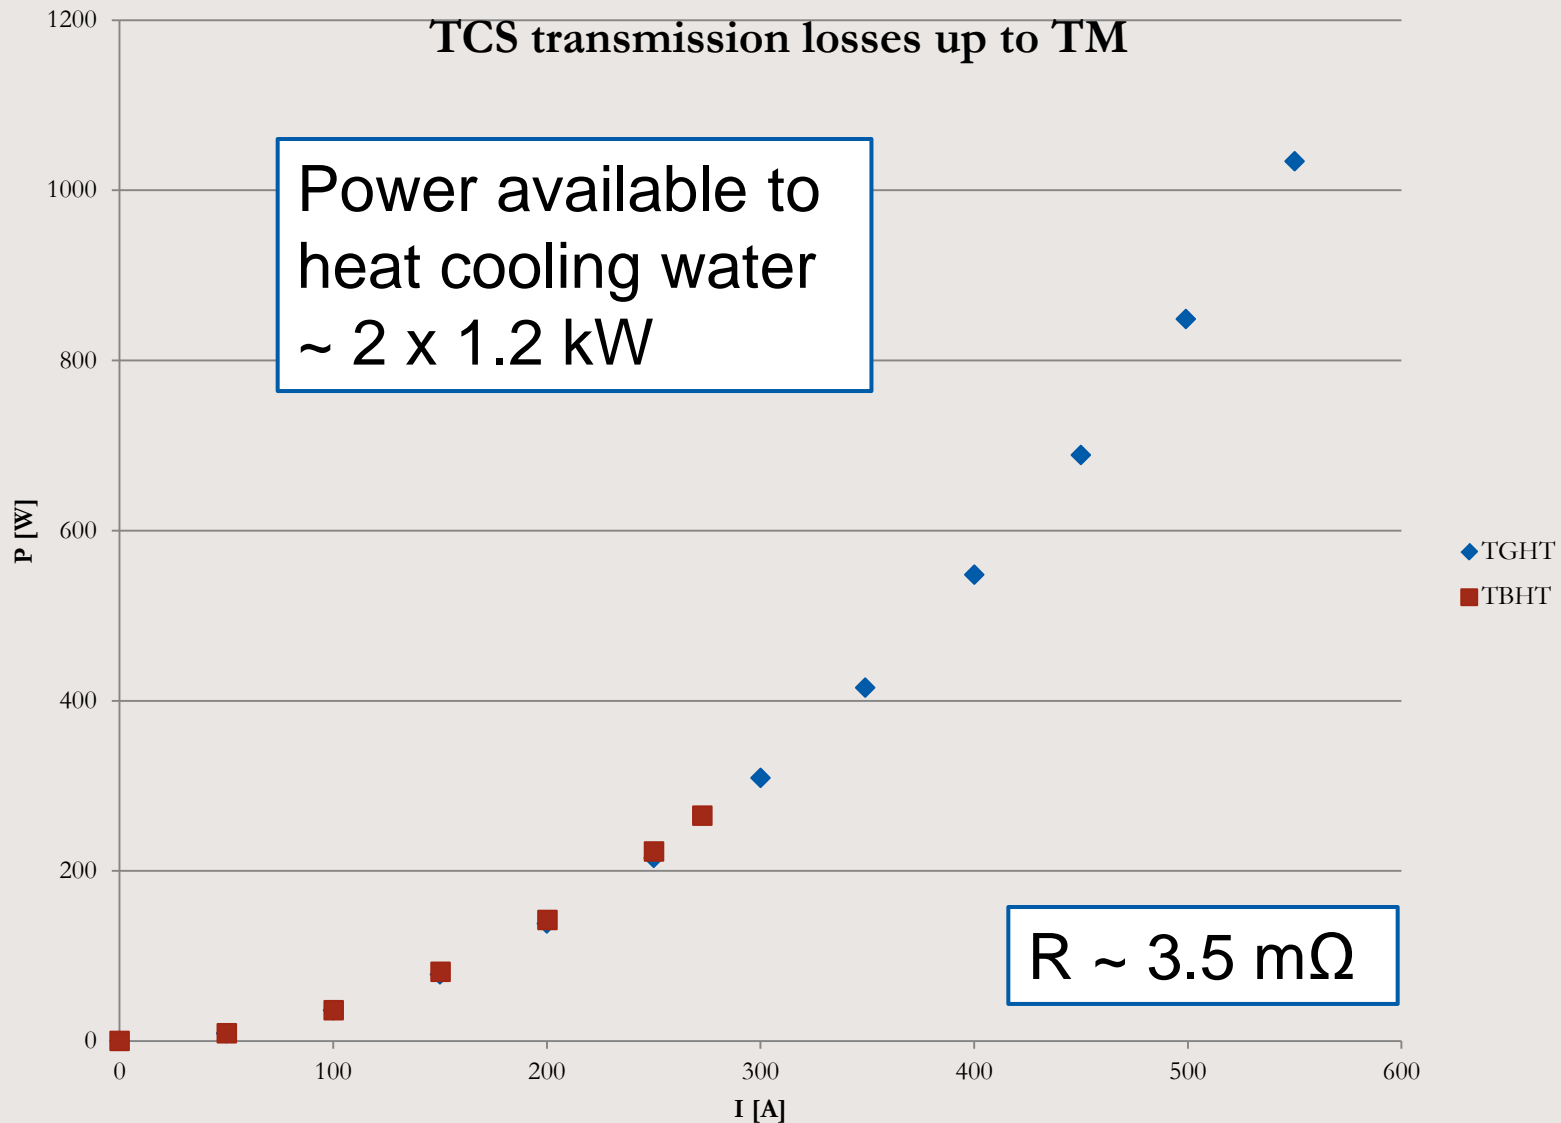

TCS Heating Test pending

- Heat from pumps brings water to ~ 32 °C
- TGHT & TBHT interlocks at 25 °C water
- Bypass/forces not fully implemented

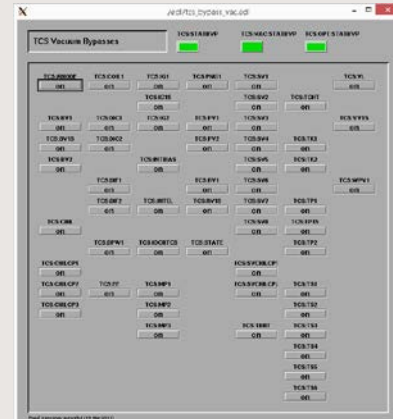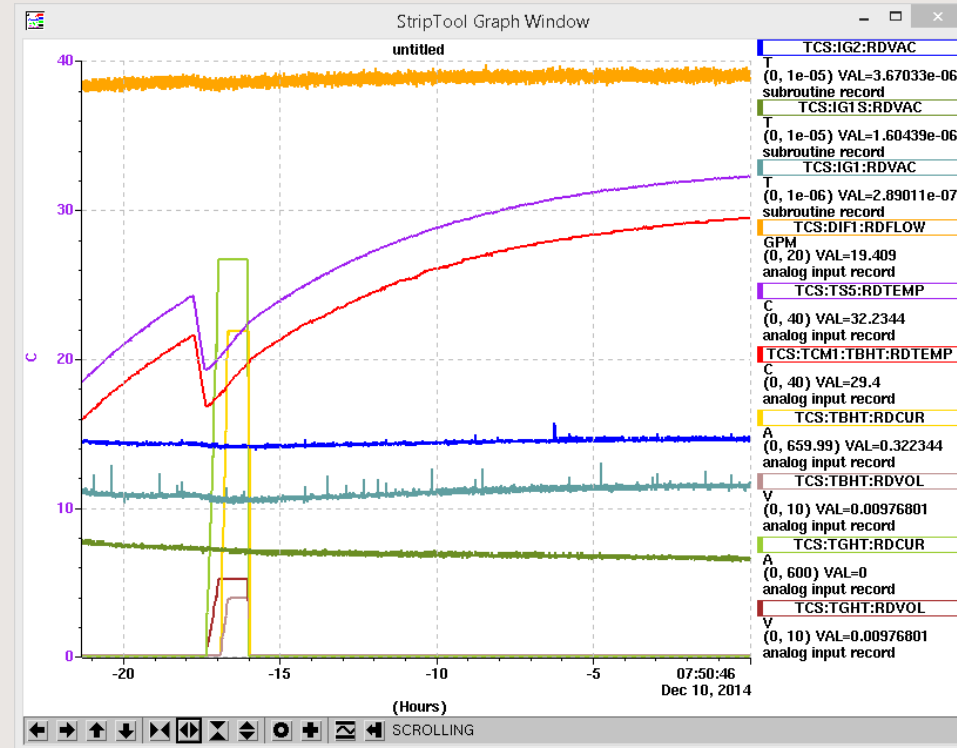

TCS Spikes of air (?)

