

A	0.0×10^{-9}
B	3.7×10^{-9}
C	1.9×10^{-9}
D	4.4×10^{-9}
PQ	7.0×10^{-9}
RU	1.8×10^{-9}
MSP	0.0×10^{-9}
EE	0.0×10^{-9}
HS	4.0×10^{-9}
WINDOW	0.0×10^{-9}


70 PSI: Argon
refilled at last

ITW Helium pressure Test
on internal water line
70 PSI; 3 min each line

Tested @ 2025-01-03
Wank

ITW

primary and secondary vacuum
vessel leak check.

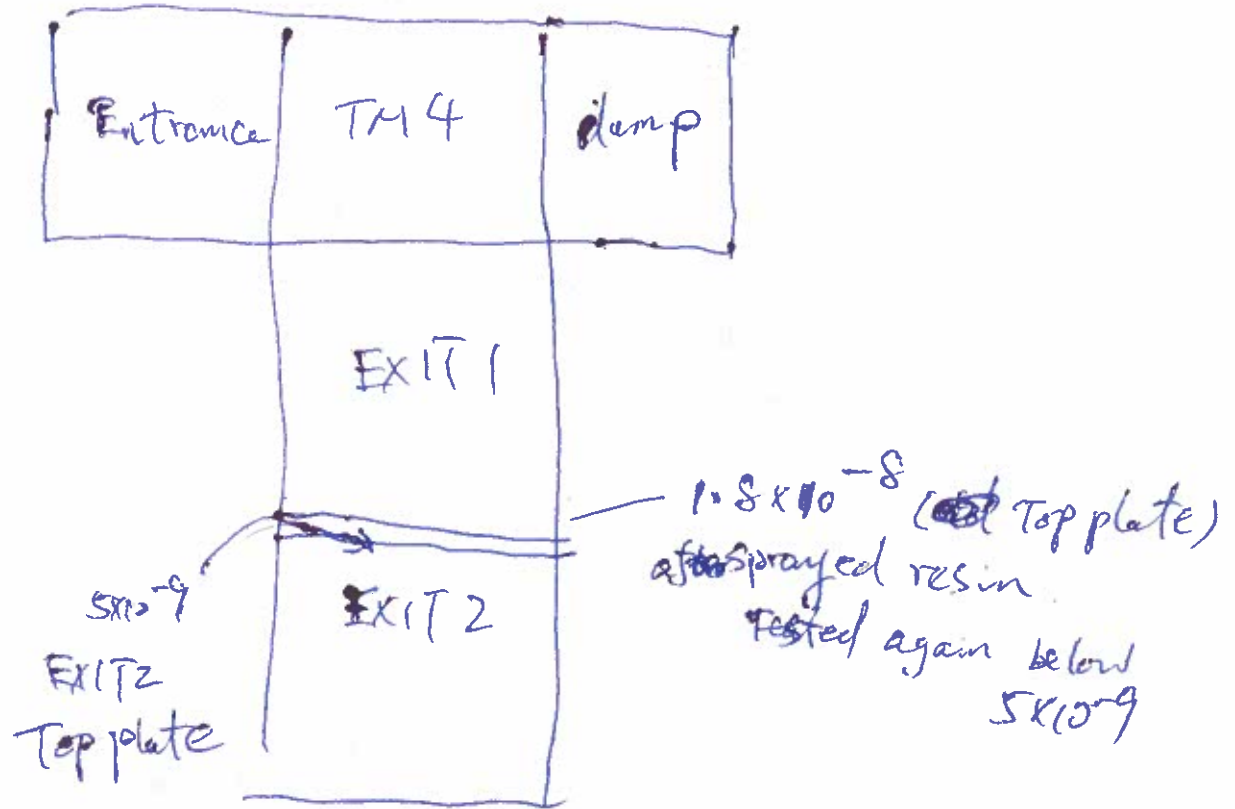

2025-01-03